



EUDAMED

funkčnosť a požiadavky na jednotlivé hospodárske subjekty

Zuzana Baťová

Štátny ústav pre kontrolu liečiv



Regulačný rámec

Regulation (EU) 2017/745 on medical devices
(MDR)

applicable since **26 May 2021**,
plus extra transitional period for ‚legacy devices‘

Regulation (EU) 2017/746 on in vitro diagnostic
medical devices (IVDR)

applicable since **26 May 2022**
plus extra transitional period for ‚legacy devices‘

EUDAMED Implementing Act
Commission Implementing
Regulation (EU) **2021/2078**

- Mode of access (restricted, public)
- Registration in EUDAMED
- Technical and administrative support

Regulation (EU) **2024/1860**

- Enable the gradual roll of the functional EUDAMED modules
- Amendment of transition periods for mandatory use of the EUDAMED modules; mandatory use of a module 6 months after publication of the notice in the *Official Journal of EU (OJEU)*



EUDAMED



- Informačný systém zriadený Nariadením (EÚ) 2017/745 a 2017/746
- Cieľom EUDAMEDu je:
 - centralizácia informácií,
 - sledovateľnosť pomôcok (UDI)
 - zvýšenie transparentnosti zlepšením prístupu k informáciám,
 - posilnenie komunikácie a koordinácie medzi stakeholdermi (CA, výrobca, dovozca, NB)
 - evidovanie incidentov a posilnenie vigilancie



Právny základ a povinnosti (1/2)

**Výrobca
Splnomocnený zástupca,
Dovozca**

sa registrujú ako „Actors“
(SRN)

Článok 31 MDR
Článok 28 IVDR

**System/Procedure Pack
Producer,**

vkladajú UDI a ostatné
údaje podľa prílohy VI

Článok 28,29 MDR
Článok 25,26 IVDR

Notifikovaná osoba

Vkladajú informácie o
certifikátoch a
žiadostiach (zamietnutie,
stiahnutie)

Článok 57 MDR
Článok 52 IVDR



Právny základ a povinnosti (2/2)

Sponzor a Kompetentná autorita

klinické skúšanie/štúdie
výkonu

Článok 73 MDR
Článok 69 IVDR

Výrobca Splnomocnený zástupca, Kompetentná autorita

vigilančné hlásenia (MIR,
FSCA) a PSUR

Článok 92 MDR
Článok 87 IVDR

Kompetentná autorita

Informácie o opatreniach
z trhového dohľadu,
inšpekčné správy,
nesúlady výrobkov

Článok 100 MDR
Článok 95 IVDR

EUDAMED landing page

The screenshot shows the EUDAMED landing page with several key elements highlighted by red boxes and arrows. On the left, two blue arrows point to the 'Sign in to EUDAMED' button and the 'Need help?' section. The 'Sign in to EUDAMED' button is located in the main content area, below the introductory text. The 'Need help?' section is located in the bottom right corner, featuring a magnifying glass icon and a link to the 'EUDAMED information center'. The 'Documents' section is located at the bottom left, listing two PDF documents: 'User's rights and obligations' and 'Declaration on information security responsibilities'. The 'Release note v 2.25.3' section is located in the top right corner, providing information about the latest version of the system. The 'Warning' section is located in the middle right, providing information about system maintenance and the mandatory use of the first four modules starting from May 28, 2026.

European Commission | EUDAMED

European Commission > EUDAMED

Welcome to EUDAMED - European Database on Medical Devices

EUDAMED is the IT system established by [Regulation \(EU\) 2017/745](#) on medical devices and [Regulation \(EU\) 2017/746](#) on in vitro diagnosis medical devices.

EUDAMED provides a living picture of the lifecycle of medical devices that are made available in the European Union (EU). It integrates different electronic systems to collate and process information about medical devices. EUDAMED aims to enhance overall transparency, including better access to information for public and healthcare professionals, and to enhance coordination between the different Member States in the EU.

EUDAMED is composed of six modules related to: actor registration, unique device identification (UDI) and device registration, notified bodies and certificates, clinical investigations and performance studies, vigilance and post-market surveillance and market surveillance.

Starting from May 28, 2026, the use of the first four modules is mandatory:

1. Actor registration,
2. UDI/Devices registration,
3. Notified Bodies and Certificates,
4. Market Surveillance.

Sign in to EUDAMED

Access to EUDAMED is restricted to users identified by their EU Login account.

You already have an EU Login account

[Enter with EU Login](#)

No EU Login account? [Create your EU Login account](#)

Warning 2026-05-04
Tuesday, 5 May 2026, 07:00 CET until 19:00 CET, EUDAMED may not be available due to maintenance reasons. We apologize for the inconvenience.

Warning 2025-11-27
The notice declaring the functionality of the first four modules has been published in the OJEU. This publication initiates a 6-month transition period. Therefore, starting from May 28, 2026, it will be mandatory to use the first four modules: Actor, UDI/devices, NBs & Certificates, and Market Surveillance

Documents

[User's rights and obligations](#) [PDF 171.41 KB]

[Declaration on information security responsibilities](#) [PDF 221.52 KB]

Need help?

[EUDAMED information center](#)

Find the answer you are looking for in the EUDAMED information centre

Vytvorený
EU login



Potreba mať
dva LAA účty
pre zaistenie
prístupu k
údajom HS



Informačné centrum EUDAMED

European Commission

Information Centre – EUDAMED

Getting started **Documentation** Actor Search by module Data exchange Frequently Asked Questions Onboarding material Sitemap

EC Health and Food Safety / Information Centre – EUDAMED / Welcome to the EUDAMED information centre

WARNING

News
Nov 27, 2025

The notice declaring the functionality of the first four modules has been published in the OJEU. This publication initiates a 6-month transition period. Therefore, starting from May 28, 2026, i...

ALL NEWS →

Welcome to the EUDAMED information centre

EUDAMED provides a living picture of the lifecycle of medical devices that are made available in the European Union (EU). It integrates different electronic systems to collate and process information from the different Member States in the EU.

EUDAMED is composed of six modules related to: actor registration, unique device identification (UDI) and device registration, notified bodies and certificates, clinical investigations and performance evaluation.

1 Starting from May 28, 2026, the use of four modules is mandatory:

1. Actor registration;
2. UDI/Devices registration;
3. Notified Bodies and Certificates;
4. Market Surveillance

Getting Started →
Get started using the EUDAMED platform, learn the basics

Documentation →
User guides, technical documentation and release notes

<https://webgate.ec.europa.eu/eudamed-help/en/welcome-to-the-eudamed-information-centre.html>

VEREJNÁ ČASŤ/ PUBLIC

The screenshot shows the public interface of the EUDAMED website. At the top left is the European Commission logo. To its right is a language selector set to 'English' and a search bar with a 'Search' button. Below this is a dark blue navigation bar with the title 'EUDAMED - European Database on Medical Devices' and a menu with items: Home, Actors, UDI/Devices, Certificates, and News. The main content area starts with a 'Home >' link, followed by the heading 'EUDAMED database'. A paragraph explains that the database is part of new EU regulations (2017/745 and 2017/746) and aims to enhance transparency. Another paragraph states that the database will be composed of six modules. Below this is a 'Search for' section with three highlighted cards: 'Economic Operators', 'Devices, Systems, Procedure packs', and 'Certificates (Issued or Refused)'. Each card contains an icon, a title, and a brief description of the search scope.

European Commission

English Search Search

EUDAMED - European Database on Medical Devices

Home Actors UDI/Devices Certificates News

Home >


EUDAMED database


The creation of a European database on medical devices (EUDAMED) is one of the key aspects of the new rules on medical devices ([Regulation \(EU\) 2017/745](#)) and in vitro diagnostic medical devices ([Regulation \(EU\) 2017/746](#)).


EUDAMED will provide a living picture of the lifecycle of medical devices that are made available in the European Union (EU). It will integrate different electronic systems to collate and process information about medical devices and related companies (e.g. manufacturers). In doing so, EUDAMED aims to enhance overall transparency, including through better access to information for the public and healthcare professionals, and to enhance coordination between the different Member States in the EU.

EUDAMED will be composed of six modules related to: actor registration, unique device identification (UDI) and device registration, notified bodies and certificates, clinical investigations and performance studies, vigilance and market surveillance.

Search for


Economic Operators
Search for economic operators (manufacturers, system/procedure pack producers, authorised representatives, importers).



Devices, Systems, Procedure packs
Search for UDI-DI and device data including SS(C)P.


Certificates (Issued or Refused)
Search for certificates and refused certificates.

<https://ec.europa.eu/tools/eudamed/#/screen/home>



Štruktúra databázy
EUDAMED

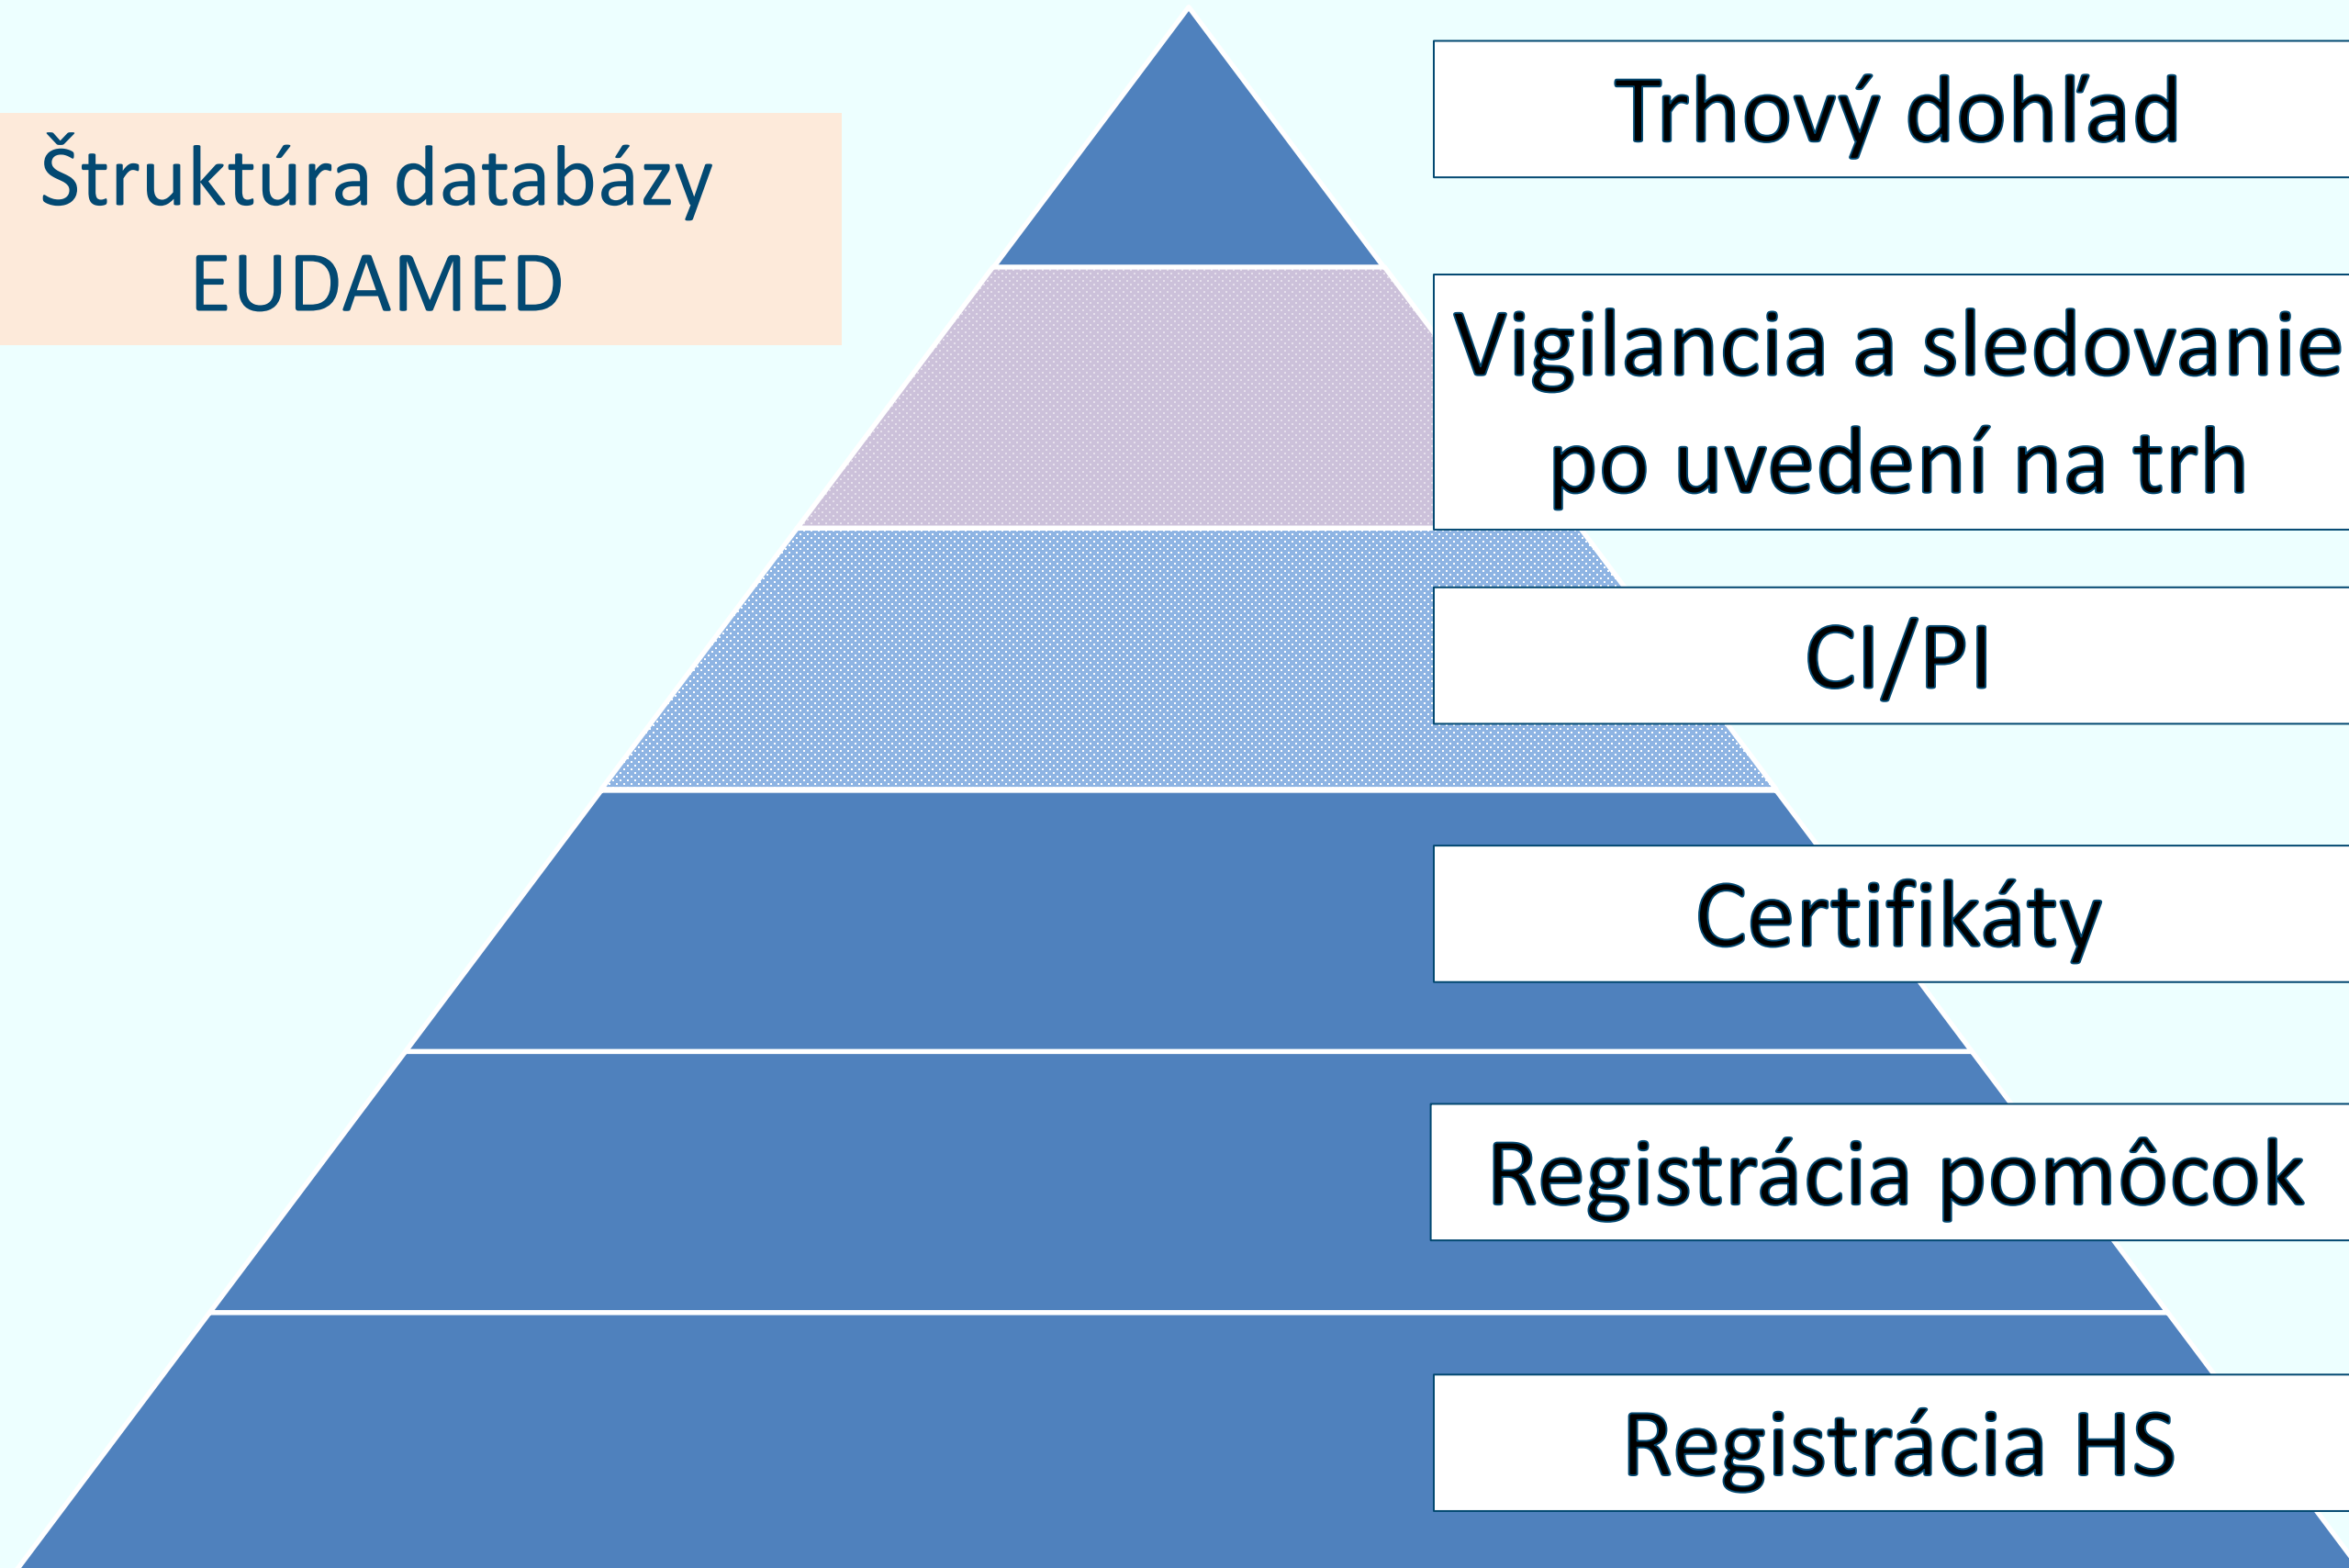

Actor/ aktívny užívateľ

organizácia/PO/FO, ktorá musí byť registrovaná v EUDAMEDe a mať doňho prístup, pretože má povinnosti vyplývajúce z MDR/IVDR ohľadom vkladania údajov, obsahu

Supervising roles/ Dohľad

- EK
- NCAs
- NBs
- Určené orgány

Economic operators´ Role/ HS

- Výrobcovia (EU a non-EU)
- Dovozcovia (EU)
- Splnomocnení zástupcovia (EU)
- Kompletizéri systémov/súprav (EU a nonEU)

Sponzor/ Zadávateľ

- Zadávatelia klinických skúšaní/štúdií výkonu

**Distribútori nie sú
v EUDAMEDe !**

Čo v EUDAMED nájdete

- Výrobcov, EC REP, Dovozcov
- ZP/IVD **sériovo vyrábané** a k nim údaje
 - Názov pomôcky
<https://ec.europa.eu/tools/eudamed/#/screen/search-device/9a1c859e-483c-4e19-860e-0e6ddc5c7c7e>
 - Basic UDI, master UDI
 - ES certifikáty
 - riziková trieda
 - EMDN kód a
 - ďalšie údaje vymedzené v časti A oddiele 1 prílohy VI MDR
- ES certifikáty

Čo v EUDAMED nenájdete

- Informácia o ZP/IVD v SK jazyku a **návod na použitie v štátnom jazyku**
- Evidencia výrobcov ZP na mieru so sídlom v SR
- Evidencia výrobcu IVD v zdravotníckych zariadeniach v SR podľa čl. 5 (5) IVDR
- Povinná registrácia distribútora, keďže distribútori sa neregistrujú v EUDAMEDe
- Hlásenia podľa čl. 16 MDR (preklady, prebaľovanie, preznačovanie)
- Hlásenia podľa čl. 10a (prerušenie alebo ukončenie dodávok ZP/IVD) (revízia nariadení uvažuje o zariadení centrálného modulu)

Registrácia hospodárskych subjektov

Výrobcovia: registrujú sa sami; registrujú svoje ZP/IVD ZP a vkladajú prislúchajúce správy z PMS a vigilancie

Dovozcovia: registrujú sa sami, priradia sa k výrobcovi mimo EÚ, pre ktorých uvádzajú ZP/IVD ZP na trh; môžu kontrolovať údaje o týchto výrobcovi mimo EÚ a výrobkoch zadaných do EUDAMED

Splnomocnení zástupcovia: registrujú sa sami; participujú na registrácii non EU výrobcov; registrujú vigilančné hlásenia (ak je to potrebné) a overujú informácie poskytnuté non-EU výrobcovi

System/procedure pack producer: registrujú sa sami a registrujú svoje systémy/súpravy



Slovenské HS sú **validované a **konfirmované** v EUDAMEDe **ŠÚKLom** → SRN**



Potrebné údaje k registrácii

- Actor role
- Organisation name
- Organisation identifiers
- Organisation address
- Authorised representative (for non-EU MF)
- Responsible CA (depending on address)
- Public contact details
- Contact details for CAs (non-public)
- PRRC (only for MF and AR)
- Signed agreement annex (non-public) (Prehlásenie o zodpovednosti za bezpečnosť informácií)
- Organisation identification document (**Výpis z OR**; pri výrobcoch činnosť „výroba ZP“)



Správne vyplnenie údajov pri registrácii hospodárskeho subjektu v EUDAMED

Registrácia hospodárskeho subjektu v EUDAMED-e pozostáva z 4 krokov:

1. Actor identification:

- **Role:**
vloďte rolu o ktorú žiadate (*Manufacturer/výrobca; Authorised Representative/splnomocnený zástupca; Importer/dovozca; System & Procedure Pack Producer/výrobca systému alebo súprav pomôcok*)
- **Country:**
vloďte *Slovakia*
- **Actor/Organisation name:**
vloďte *názov spoločnosti*
- **VAT number:**
vloďte *IČ DPH*
- **National trade register number:**
vloďte *IČO*
- **Organisation identification document:**
vloďte *výpis z obchodného registra (pri výrobcoch činnosť „výroba ZP“)*

STEP 1 Actor Identification	
Role:	Vloďte rolu o ktorú žiadate (výrobca/manufacturer; dovozca/importer; splnomocnený zástupca/EC REP...)
Country:	Slovakia
Actor / Organisation name:	Vloďte názov spoločnosti
Abbreviated name:	-
VAT information:	Yes
VAT number:	Vloďte DIČ
EORI number:	-
National trade register number:	Vloďte IČO
Organisation identification document:	Vloďte výpis z obchodného registra
Last confirmation date:	-

2. Actor address:

Vyplňte potrebné údaje ako ulica, popisné číslo, mesto, PSČ

3. Actor contact details:

Vloďte kontaktné a funkčné údaje

4. Registering Local Actor Administrator:

- Vyplňte požadované údaje

- Stiahnite si na odkaze nižšie dokument s názvom "Declaration on Information Security Responsibilities in the Context of the European Medical Device Database/ Vyhlásenie o zodpovednosti za bezpečnosť informácií v súvislosti s Európskou databázou zdravotníckych pomôcok)"

SK verzia

https://health.ec.europa.eu/document/download/6940d07d-ce39-42b2-a9bb-eb1ac352ffbe_sk

EN verzia

<https://webgate.ec.europa.eu/eudamed-static/documents/assets/responsibilities/WEB-2020-00306-01-06-EN-TRA-00%20july.pdf>

Vyplňte Vyhlásenie s tým, že v dokumente označíte rolu o ktorú žiadate a ktorá musí korešpondovať s rolou o ktorú žiadate v kroku 1. Podpíšte a vložte dokument do políčka "Signed declaration".



Toto je pilotná verzia nového webu. Predchádzajúcu verziu nájdete na povodny.sukl.sk

Oficiálna stránka verejnej správy SR

SUKL Štátny ústav pre kontrolu liečiv

Zadajte hľadaný výraz

O nás

[Domov](#) > [Pre odborníkov a firmy](#) > [Zdravotnícke pomôcky](#)

Aktuality

Obsah pripravujeme

Aktívne pracujeme na doplnení obsahu pre túto stránku. Ďakujeme za trpezlivosť.

Aktuality

[Správne vyplnenie údajov pri registrácii hospodárskeho subjektu v EUDAMED](#)

Pri registrácii hospodárskeho subjektu v databáze EUDAMED je Štátny ústav pre kontrolu liečiv povinný validovať a potvrdiť vložené údaje a priložené dokumenty. Správne a úplné...

28.04.2026

[Pokyn ŠÚKL k registrácii v EUDAMED-e a aktualizácii údajov v národnej databáze](#)

V súvislosti s uvedením databázy EUDAMED do plnej prevádzky upozorňujeme, že **od 28. mája 2026 je registrácia hospodárskych subjektov ako aj pomôcok v databáze...**



15.04.2026 — Aktualita

[Upozornenie na aktualizáciu „MP 148 Postup pre vystavenie Certifikátu voľného predaja“ a novelizáciu tlačiva žiadosti o certifikát](#)

[Oznámenie o posielaní Informácie o vybavení žiadosti namiesto potvrdeného formulára](#)

SRN – Single Registration Number

skratka role

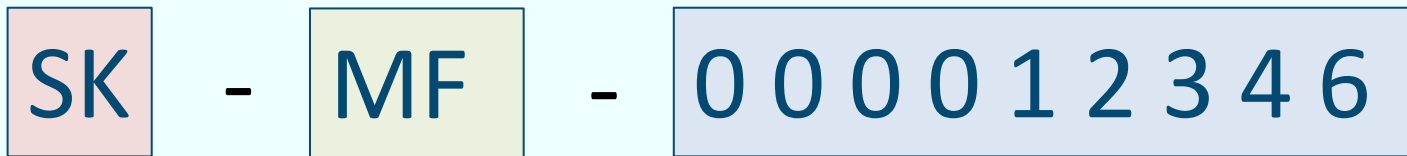

kód krajiny

9 číslic

SK-AR-
SK-IM-
SK-MF-

Home > Economic Operators

Economic Operators

The search for economic operators allows you to search and retrieve all records that contain the search terms you enter. At least one search criterion is mandatory.

Search criteria

Country: Slovakia × [New search](#)

182 records found.

Actor ID/SRN	Version	Role	Name	Abbreviated name	City name	Country	View detail
SK-MF-000001473	1 (Current)	Manufacturer	Cryomed Manufacture s.r.o. [SK]		Nové Zámky	Slovakia	View detail
SK-IM-000049887	1 (Current)	Importer	Teleflex Medical, s.r.o. [SK]		Piešťany	Slovakia	View detail
SK-IM-000049879	1 (Current)	Importer	CHONS s.r.o. [SK]	CHONS [SK]	Košice	Slovakia	View detail
SK-IM-000049812	1 (Current)	Importer	MEDICAL AiD, s.r.o. [SK]		Bratislava	Slovakia	View detail
SK-IM-000049780	1 (Current)	Importer	MG - Slovakia s.r.o. [SK]		Stará Turá	Slovakia	View detail
SK-IM-000049409	1 (Current)	Importer	Celimed s.r.o. [SK]	Celimed [SK]	Bratislava	Slovakia	View detail
SK-IM-000049003	1 (Current)	Importer	EuDent, Ltd. [SK]		Trencin	Slovakia	View detail



CURRENT ACTOR: Competent Authority, SK-CA-012, Štátny ústav pre kontrolu liečiv / State Institute for Drug Control (Slovak CA) [Slovakia] [Notifications](#)

Actor registration management



Congratulations. You have successfully assessed the actor registration.

The application ID is APP000071433

The assessment status is Registered and the Actor ID/SRN **UK-MF-000050018** has been assigned to the actor

Role:

Manufacturer

Actor / Organisation name:

Abtech Safety

Address:

Unit 38, Drive B, First Avenue, Deeside Industrial Estate, Flintshire, Deeside, **United Kingdom** (excl. Northern Ireland)


What do you want to do now?

[View pending requests](#)

[View the assessed request](#)



The EUDAMED system -
structure

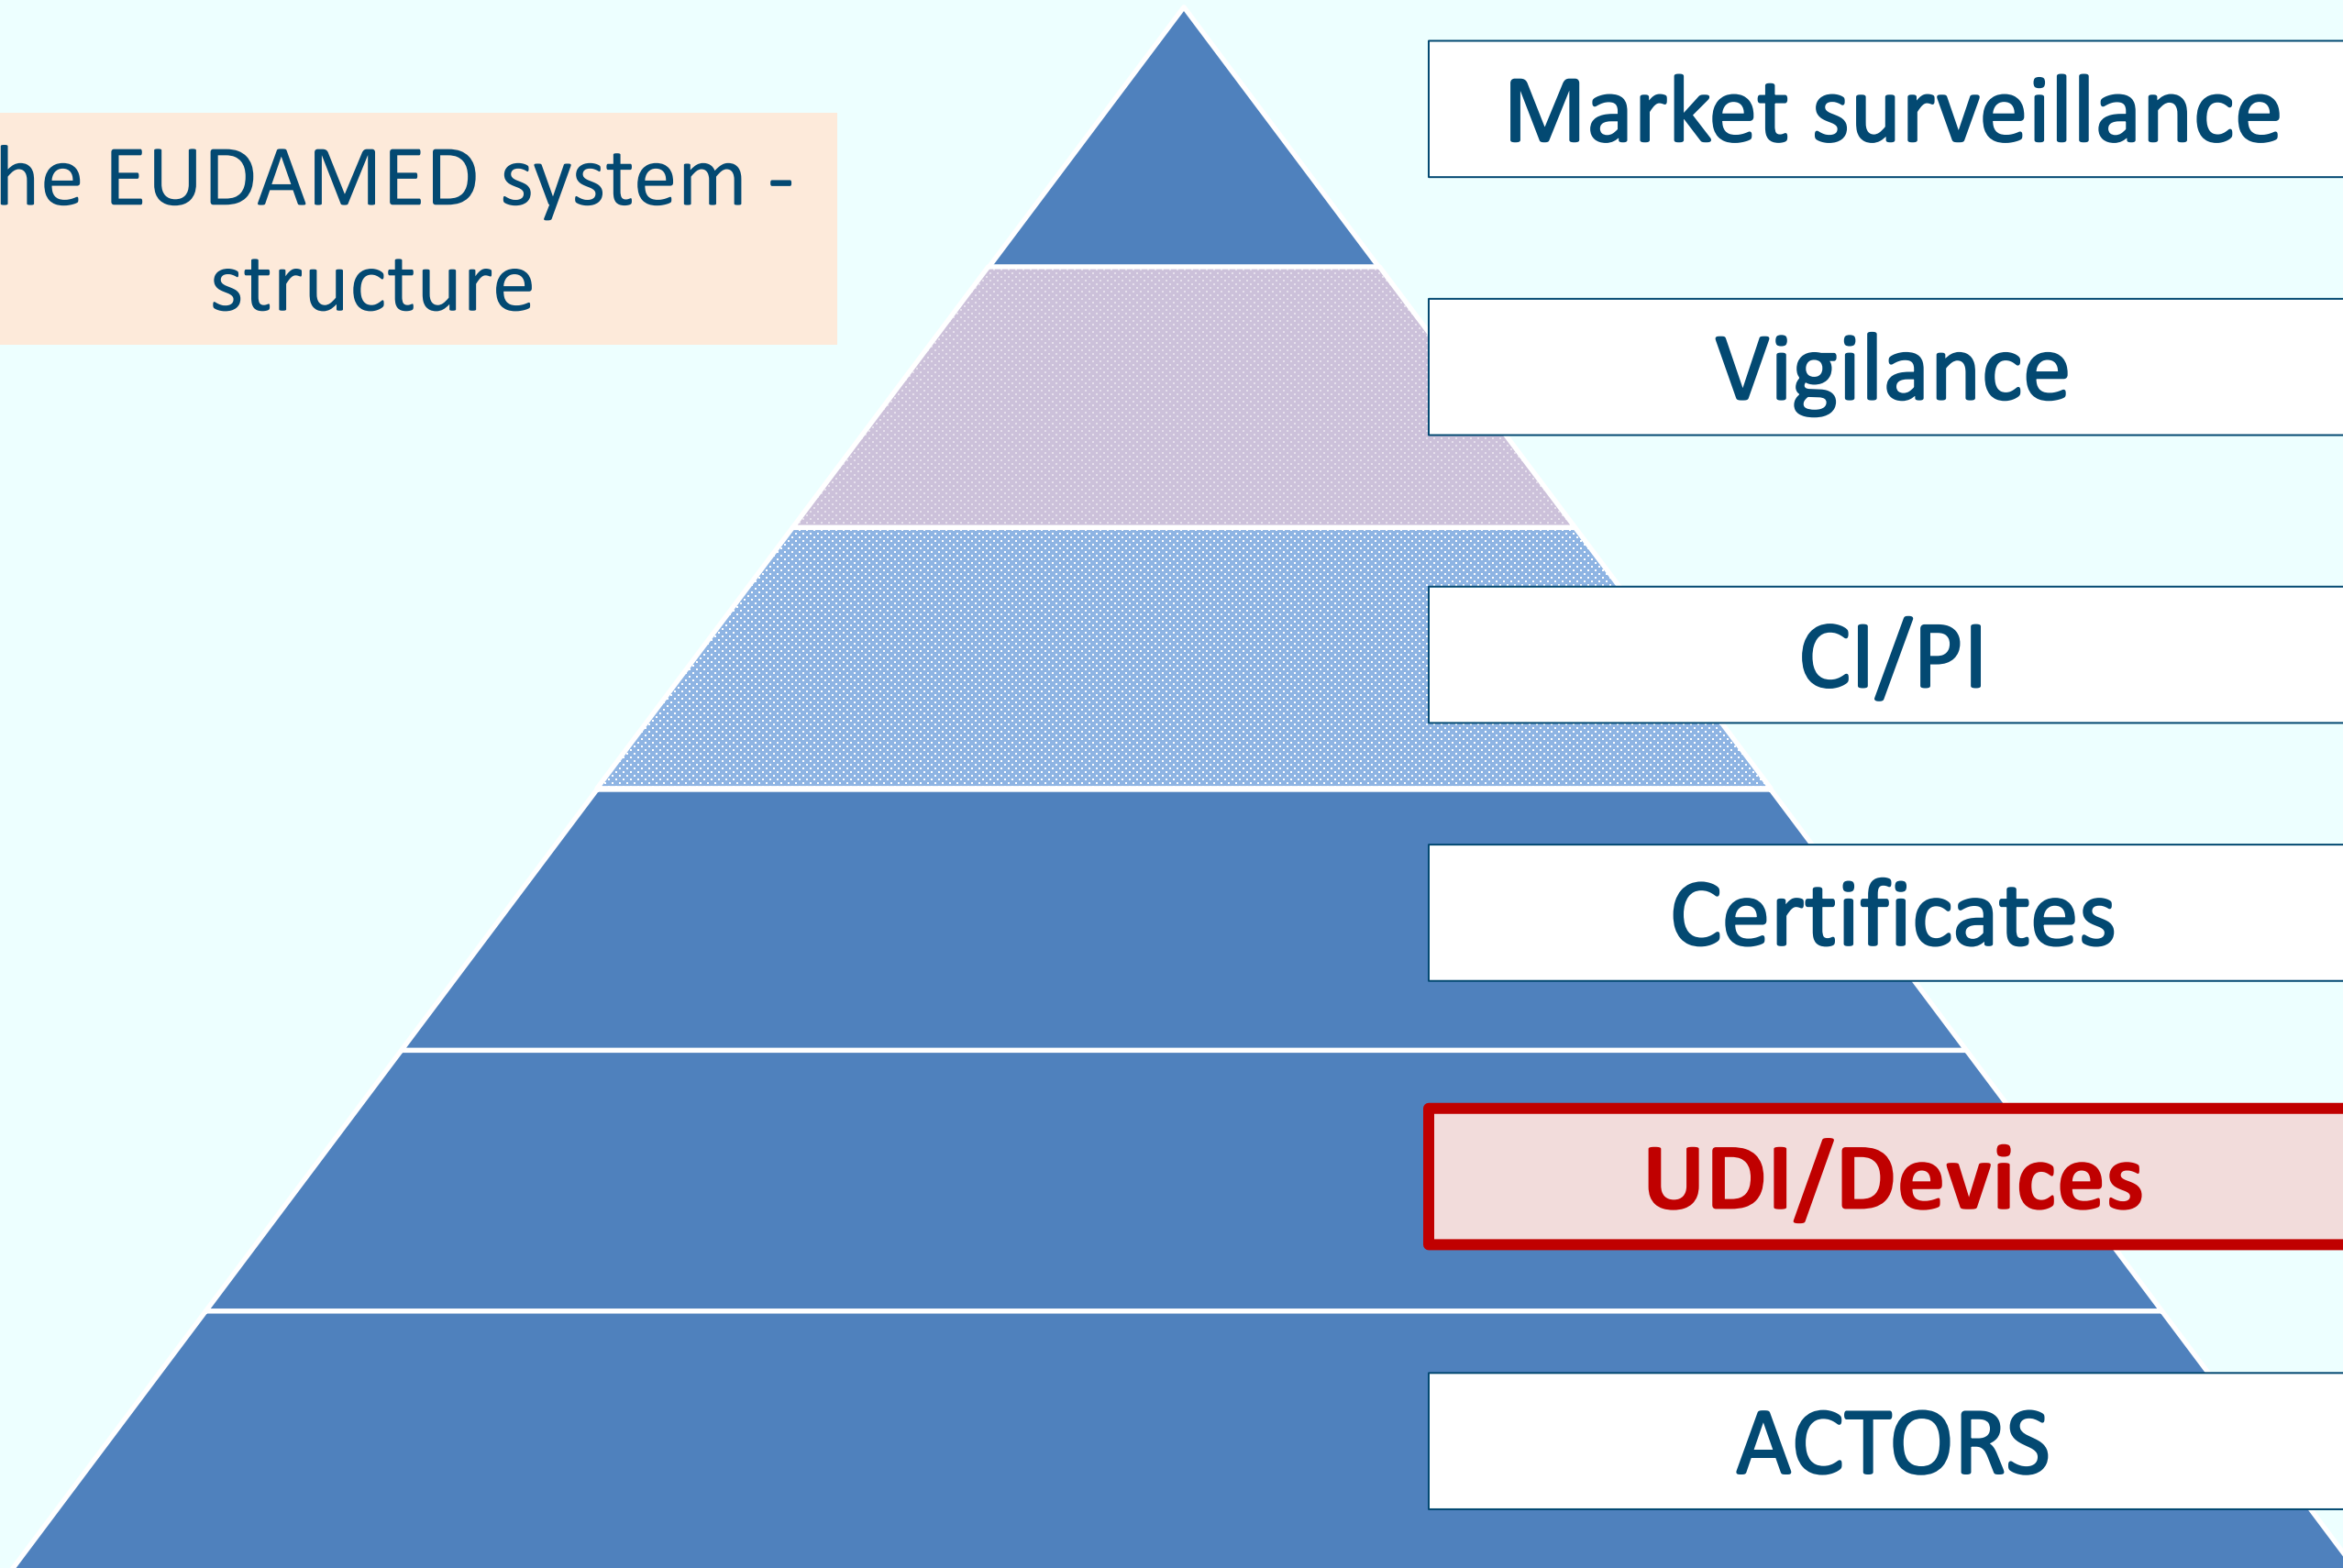



Terminológia

OLD device

ZP umiestnené na trh podľa smerníc alebo pred tým, ktorých posledná predajná jednotka (sales unit) bola uvedená na trh pred účinnosťou MDR/IVDR

LEGACY device



ZP umiestnené na trh v súlade so smernicami, ktorých jednotlivé predajné jednotky (sales unit) sú uvádzané na trh po účinnosti MDR/IVDR

REGULATION device

ZP umiestnené na trh v súlade s požiadavkami MDR/IVDR (po účinnosti MDR/IVDR)

Prechodné obdobia

Nariadenie Európskeho parlamentu a Rady (EÚ) 2023/607 a 2024/1860, ktorým sa menia nariadenia (EÚ) 2017/745 a (EÚ) 2017/746, pokiaľ ide o prechodné ustanovenia pre určité ZP a IVD ZP

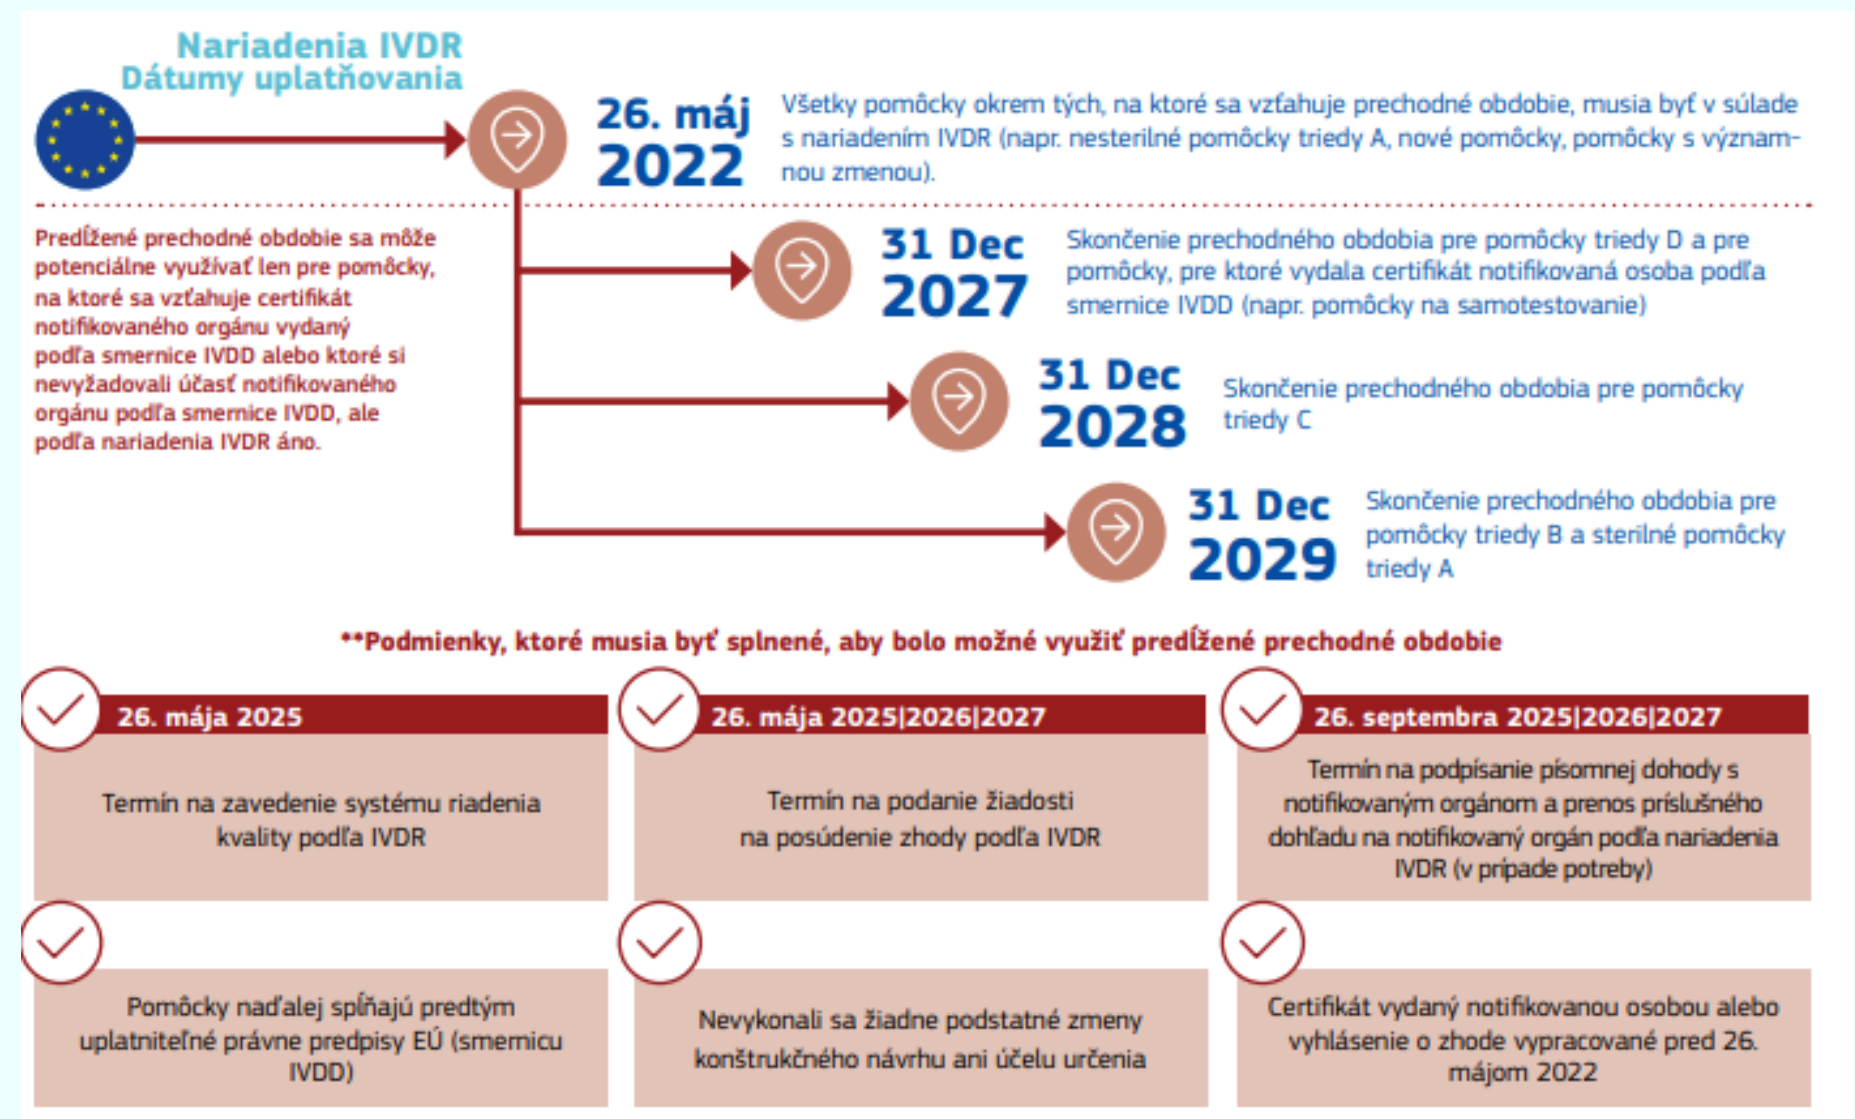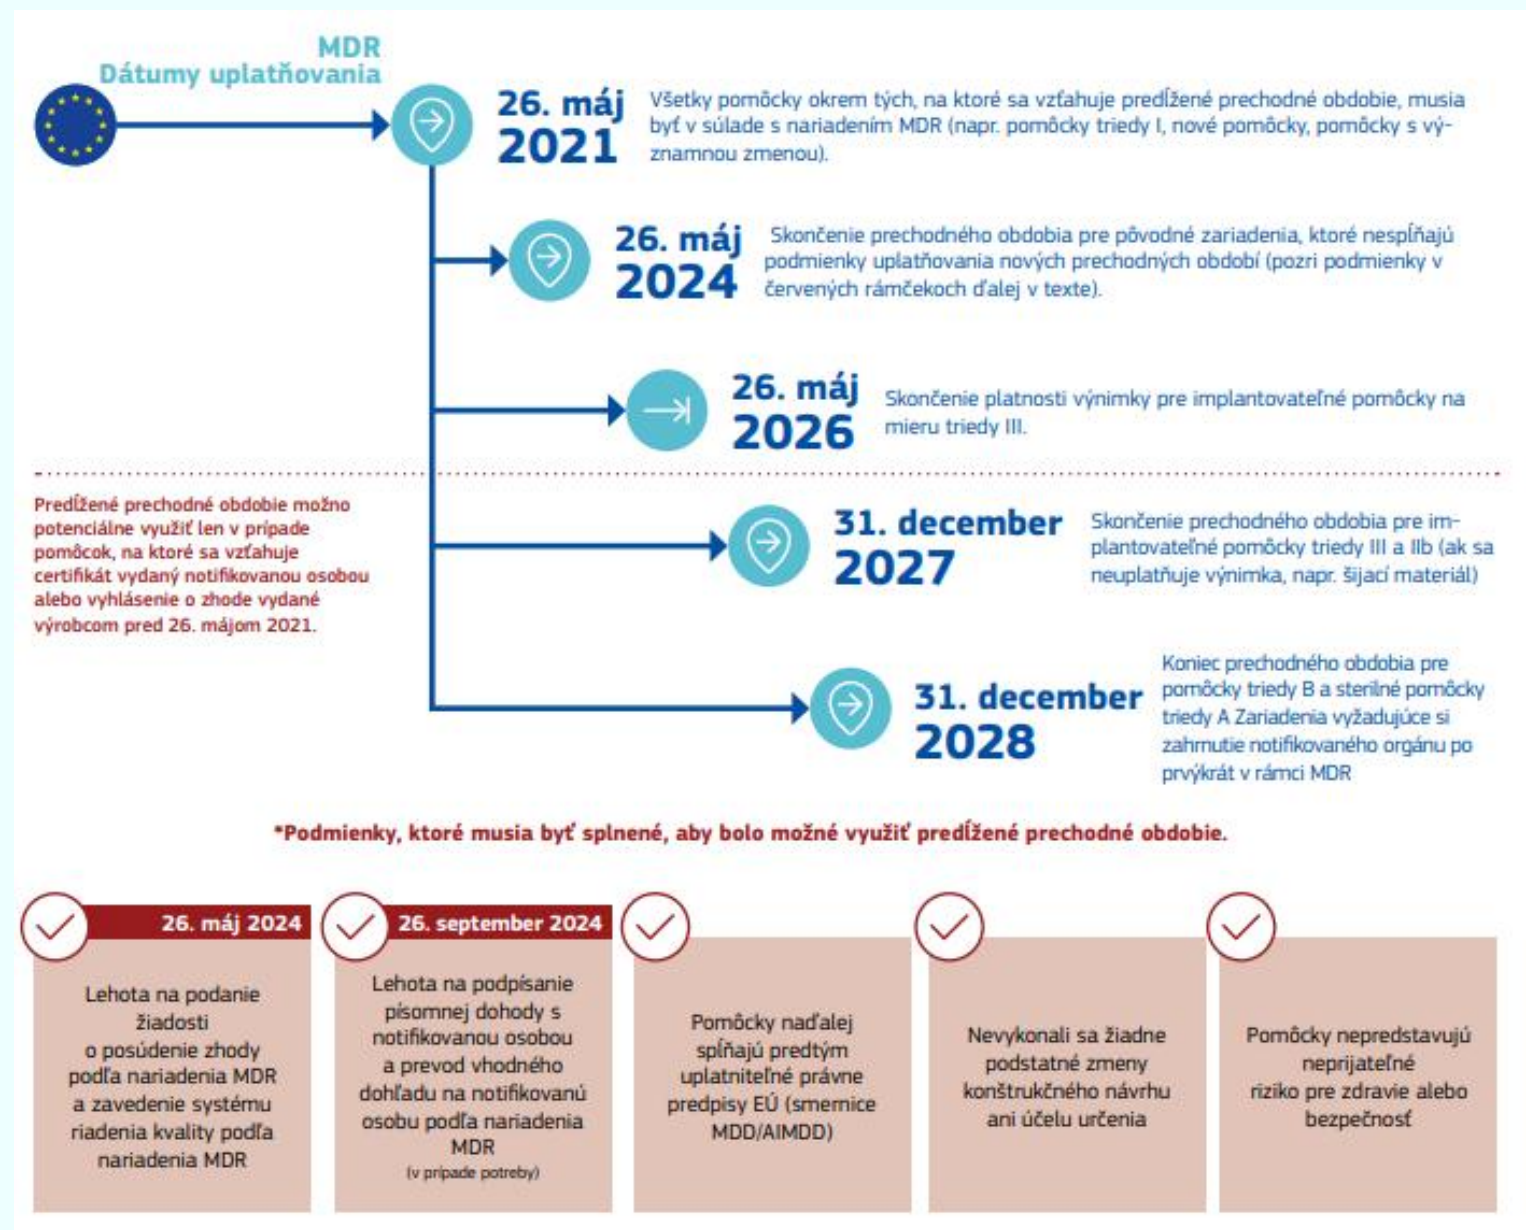


Prechodné obdobia pre všeobecné ZP

Dátum	Pravidlo	
26. máj 2021	začiatok platnosti MDR; všetky ZP, okrem tých ktoré sú uvedené nižšie, musia byť v súlade s MDR	
26. máj 2024	koniec prechodného obdobia pre legacy device ktoré nespĺňajú podmienky na aplikovanie prechodného obdobia	
26. máj 2026	koniec prechodného obdobia pre implantovateľné ZP na mieru trieda III	podaná žiadosť na NB 26.5.2024 a podpísaná zmluva s NB do 26.9.2025
31. december 2027	koniec prechodného obdobia pre implantovateľné ZP trieda III a IIb	
31. december 2028	koniec prechodného obdobia pre ostatné triedy IIb, IIa, I sterilné/s meracou funkciou	

Prechodné obdobia pre diagnostické ZP *in vitro*

Dátum	Pravidlo	
26. máj 2022	začiatok platnosti IVDR; všetky IVD, okrem tých ktoré sú uvedené nižšie, musia byť v súlade s IVDR	
26. máj 2025	koniec prechodného obdobia pre legacy device ktoré nespĺňajú podmienky na aplikovanie prechodného obdobia	
31. december 2027	koniec prechodného obdobia pre triedu D (pokiaľ išlo o IVD ostatné) a pre IVD s certifikátom vydaným NB podľa IVDD (príloha II zoznam A, príloha II zoznam B, self-testing)	podaná žiadosť na NB 26.5.2025 a podpísaná zmluva s NB do 26.9.2025
31. december 2028	koniec prechodného obdobia pre triedu C (pokiaľ išlo o IVD ostatné)	podaná žiadosť 26.5.2026 a podpísaná zmluva do 26.9.2026
31. december 2029	koniec prechodného obdobia pre triedu B a A sterilné (pokiaľ išlo o IVD ostatné)	podaná žiadosť 26.5.2027 a podpísaná zmluva do 26.9.2027

Gradual roll out and timeline

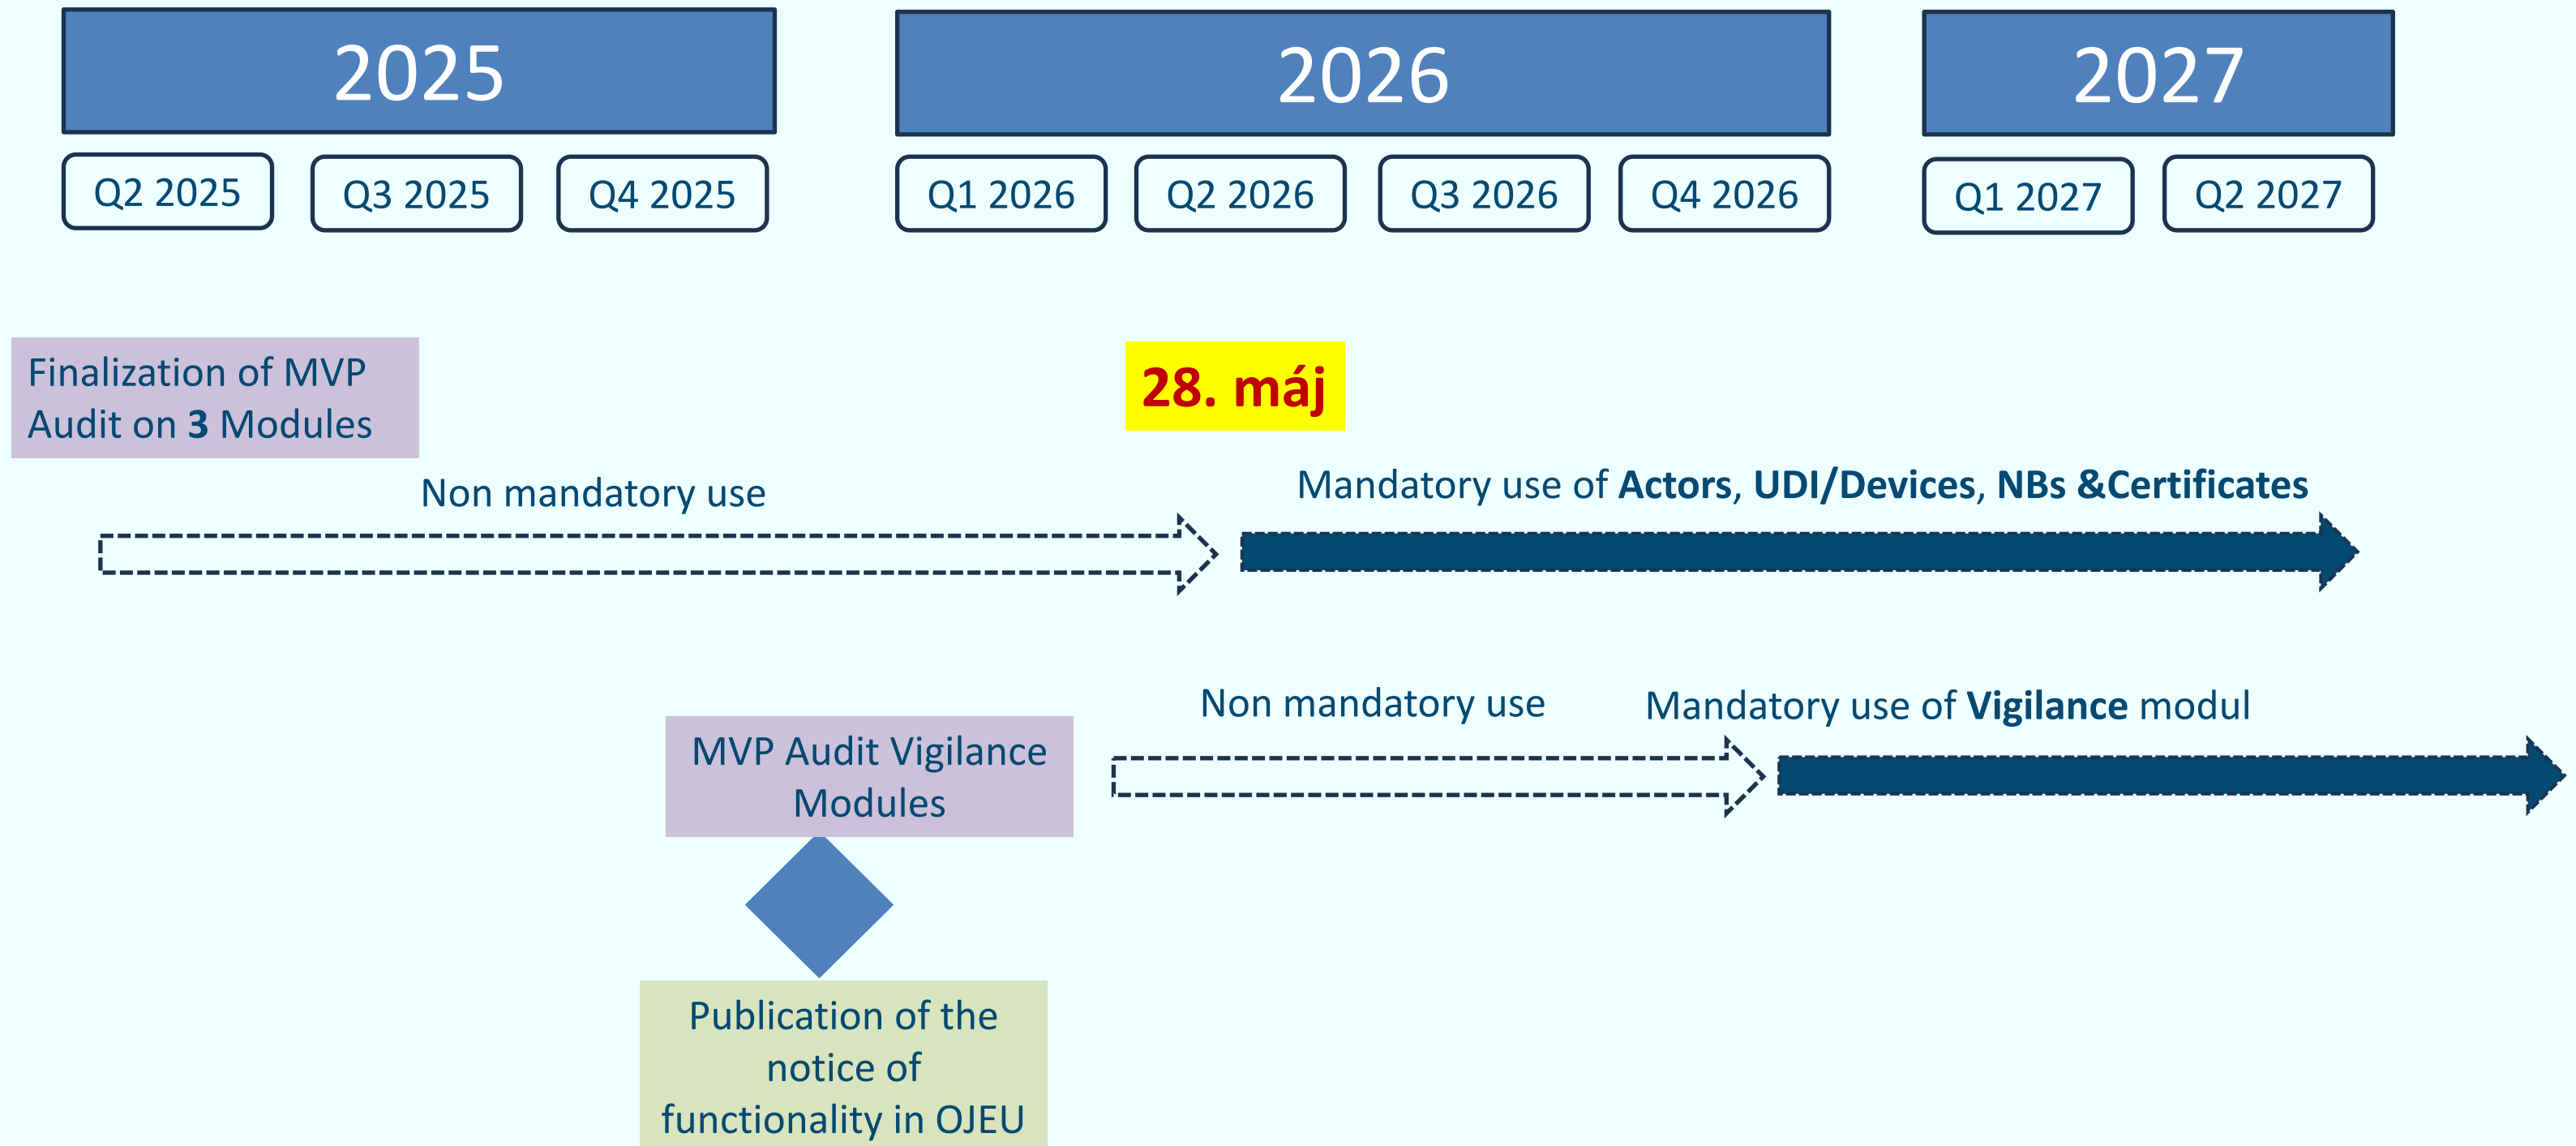

Informácie o pomôcke v EUDAMED

1. Detaily o Výrobcovi

2. BASIC-UDI-DI

- Riziková trieda
- Názov pomôcky
- Implantovateľná/ s meracou funkciou/ aktívna/ na opakované použitie
- Prítomnosť tkanív/buniek ľudského pôvodu alebo živočíšneho pôvodu

3. Certifikáty

4. UDI-DI detaily

- EMDN kód
- Obchodný názov pomôcky
- Katalógové číslo
- Veľkosti, rozmery

5. Klinické údaje (referencia na CI/PI; krajiny)

6. Distribúcia na trhu

Home > Devices/SPPs > 89043812010659

UDII UDI-DI: 89043812010659


[Go back to the list](#)

Manufacturer details [bez názvu]

Version 1 (Current) | 📅 Last update date: 2021-06-30

Actor ID/SRN	IN-MF-000008912 🔗
Role	Manufacturer
Country	India
Organisation name	INDUS MEDICARE PRIVATE LIMITED [EN]
Address	1-10-60/3, BEGUMPET (SP Road) , 500016, HYDERABAD, NA
Telephone number	+91 40 2776 2603
Email	indusmedicare.hyd@gmail.com

Identifikátory pomôcok

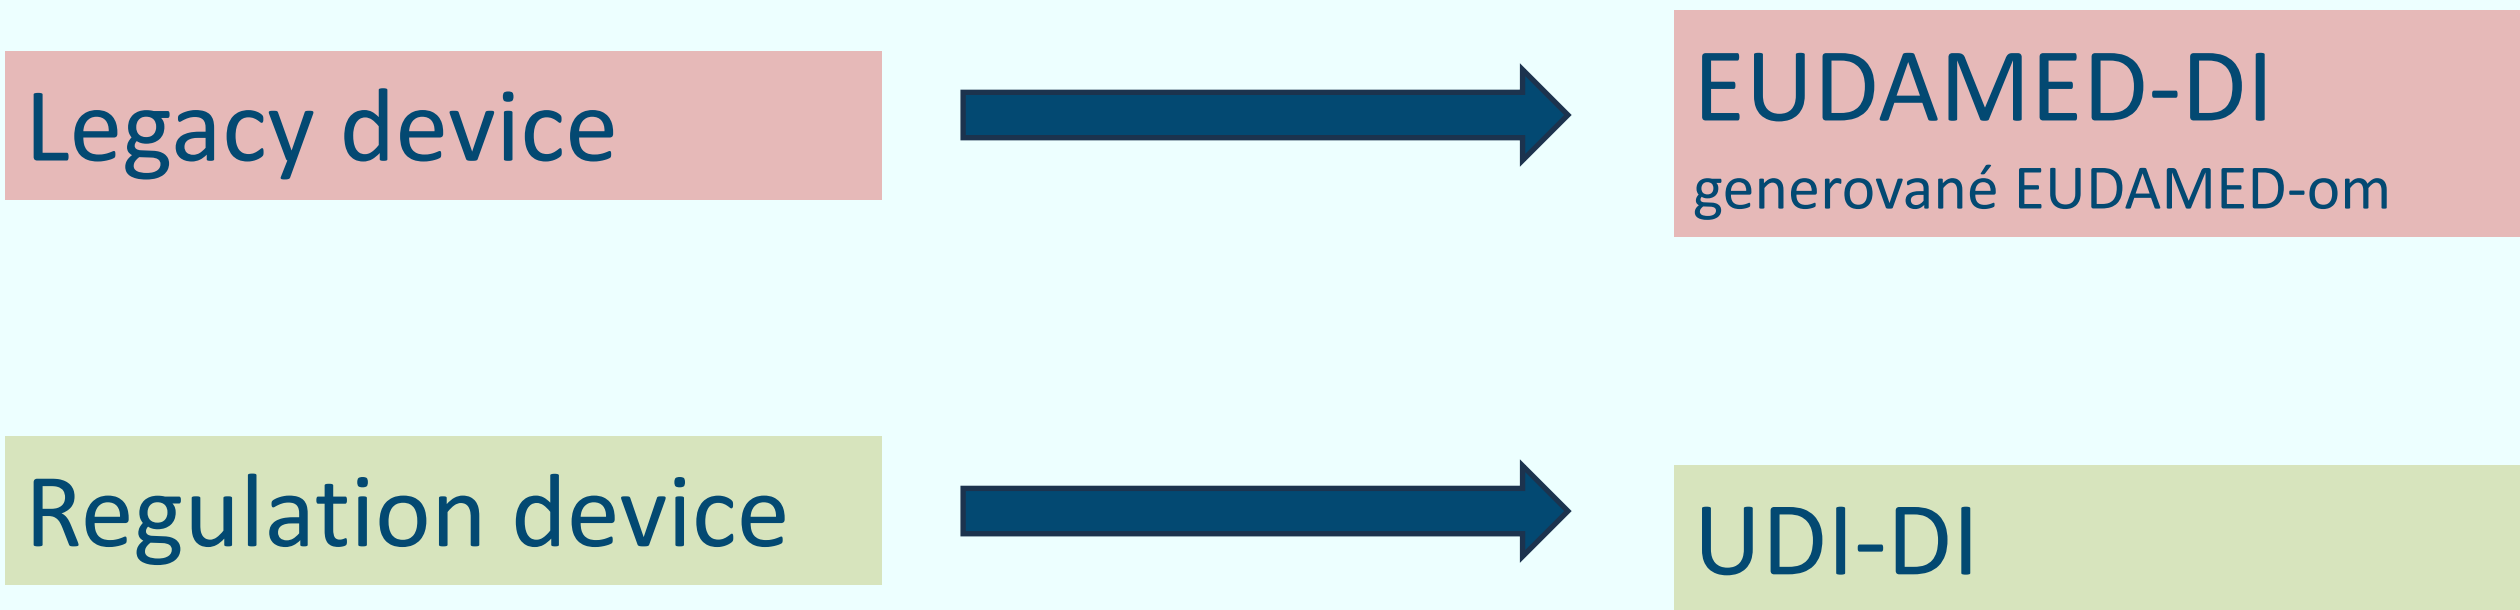

Podľa MDR/IVDR všetky pomôcky registrované v EUDAMEDe majú mať základné/basic UDI-DI.

Legacy device však podľa smerníc nemusia mať pridelené basic UDI-DI a na ich registráciu v EUDAMEDe sa preto zaviedol EUDAMED-DI.

Databáza ŠÚKL

Kategorizačný zoznam

EUDAMED master UDI-DI

60 SUKL kodov

6 SUKL kodov

9

Search criteria

Model/Name: stérilux x

Status: On the EU market x

[New search](#)

9 records found.

(Master) UDI-DI / EUDAMED ID ↓	Version	Basic UDI-DI/ EUDAMED DI	Trade name	Risk class	Manufacturer/Producer (and Authorised Representative) name	Actor ID/SRN	View detail
03261481000058	1 (Current)	32614810824C	Stérilux® ES	Class I	Laboratoires PAUL HARTMANN S. à.r.l	FR-MF-000004029	
03261481000034	1 (Current)	32614810824C	Stérilux® ES	Class I	Laboratoires PAUL HARTMANN S. à.r.l	FR-MF-000004029	
03261481000027	1 (Current)	32614810824C	Stérilux® ES	Class I	Laboratoires PAUL HARTMANN S. à.r.l	FR-MF-000004029	
03261480000394	1 (Current)	32614810824C	Stérilux® ES	Class I	Laboratoires PAUL HARTMANN S. à.r.l	FR-MF-000004029	
03261480000356	1 (Current)	32614810824C	Stérilux® ES	Class I	Laboratoires PAUL HARTMANN S. à.r.l	FR-MF-000004029	
03261480000318	1 (Current)	32614810824C	Stérilux® ES	Class I	Laboratoires PAUL HARTMANN S. à.r.l	FR-MF-000004029	
03261480000271	1 (Current)	32614810824C	Stérilux® ES	Class I	Laboratoires PAUL HARTMANN S. à.r.l	FR-MF-000004029	
03261480000233	1 (Current)	32614810824C	Stérilux® ES	Class I	Laboratoires PAUL HARTMANN S. à.r.l	FR-MF-000004029	
03261480000196	1 (Current)	32614810824C	Stérilux® ES	Class I	Laboratoires PAUL HARTMANN S. à.r.l	FR-MF-000004029	

Items per page:

50

1 – 9 of 9

⏪ ⏩

Page number:

1

Manufacturer details**Basic UDI-DI details****Certificates****UDI-DI details****Market distribution****Container Package(s)
Information**

UDI-DI code / Issuing entity	03261481000058 GS1
Status	On the EU market
UDI-DI from another entity (secondary)	-
Nomenclature code(s)	M020199: Cotton gauzes - other
Name/Trade name(s)	Stérilux® ES [FR]
Reference / Catalogue number	205027
Direct marking DI	No
i Quantity of device	1
Type of UDI-PI	Lot or batch ----- Manufacturing date ----- Expiry date
Additional Product description	Nature care Cotton Gauze 17 threads, 8 ply. [EN]
Additional information url	-
Clinical sizes	(Type): Length, (Precision): Text, (Text): 7,5 x 7,5 cm ----- (Type): Width, (Precision): Text, (Text): 7,5 x 7,5 cm
Labelled as single use	Yes
Need for sterilisation before use	No


UDI-DI details

Version 1 (Current) | 📅 Last update date: 2024-05-28


UDI-DI code / Issuing entity	03261481000034 GS1
Status	On the EU market
UDI-DI from another entity (secondary)	-
Nomenclature code(s)	M020199: Cotton gauzes - other
Name/Trade name(s)	Stérilux® ES [FR]
Reference / Catalogue number	205028
Direct marking DI	No
i Quantity of device	1
Type of UDI-PI	Lot or batch ----- Manufacturing date ----- Expiry date
Additional Product description	Nature care Cotton Gauze 17 threads, 8 ply. [EN]
Additional information url	-
Clinical sizes	(Type): Length, (Precision): Text, (Text): 7,5 x 7,5 cm ----- (Type): Width, (Precision): Text, (Text): 7,5 x 7,5 cm



The EUDAMED system -
structure

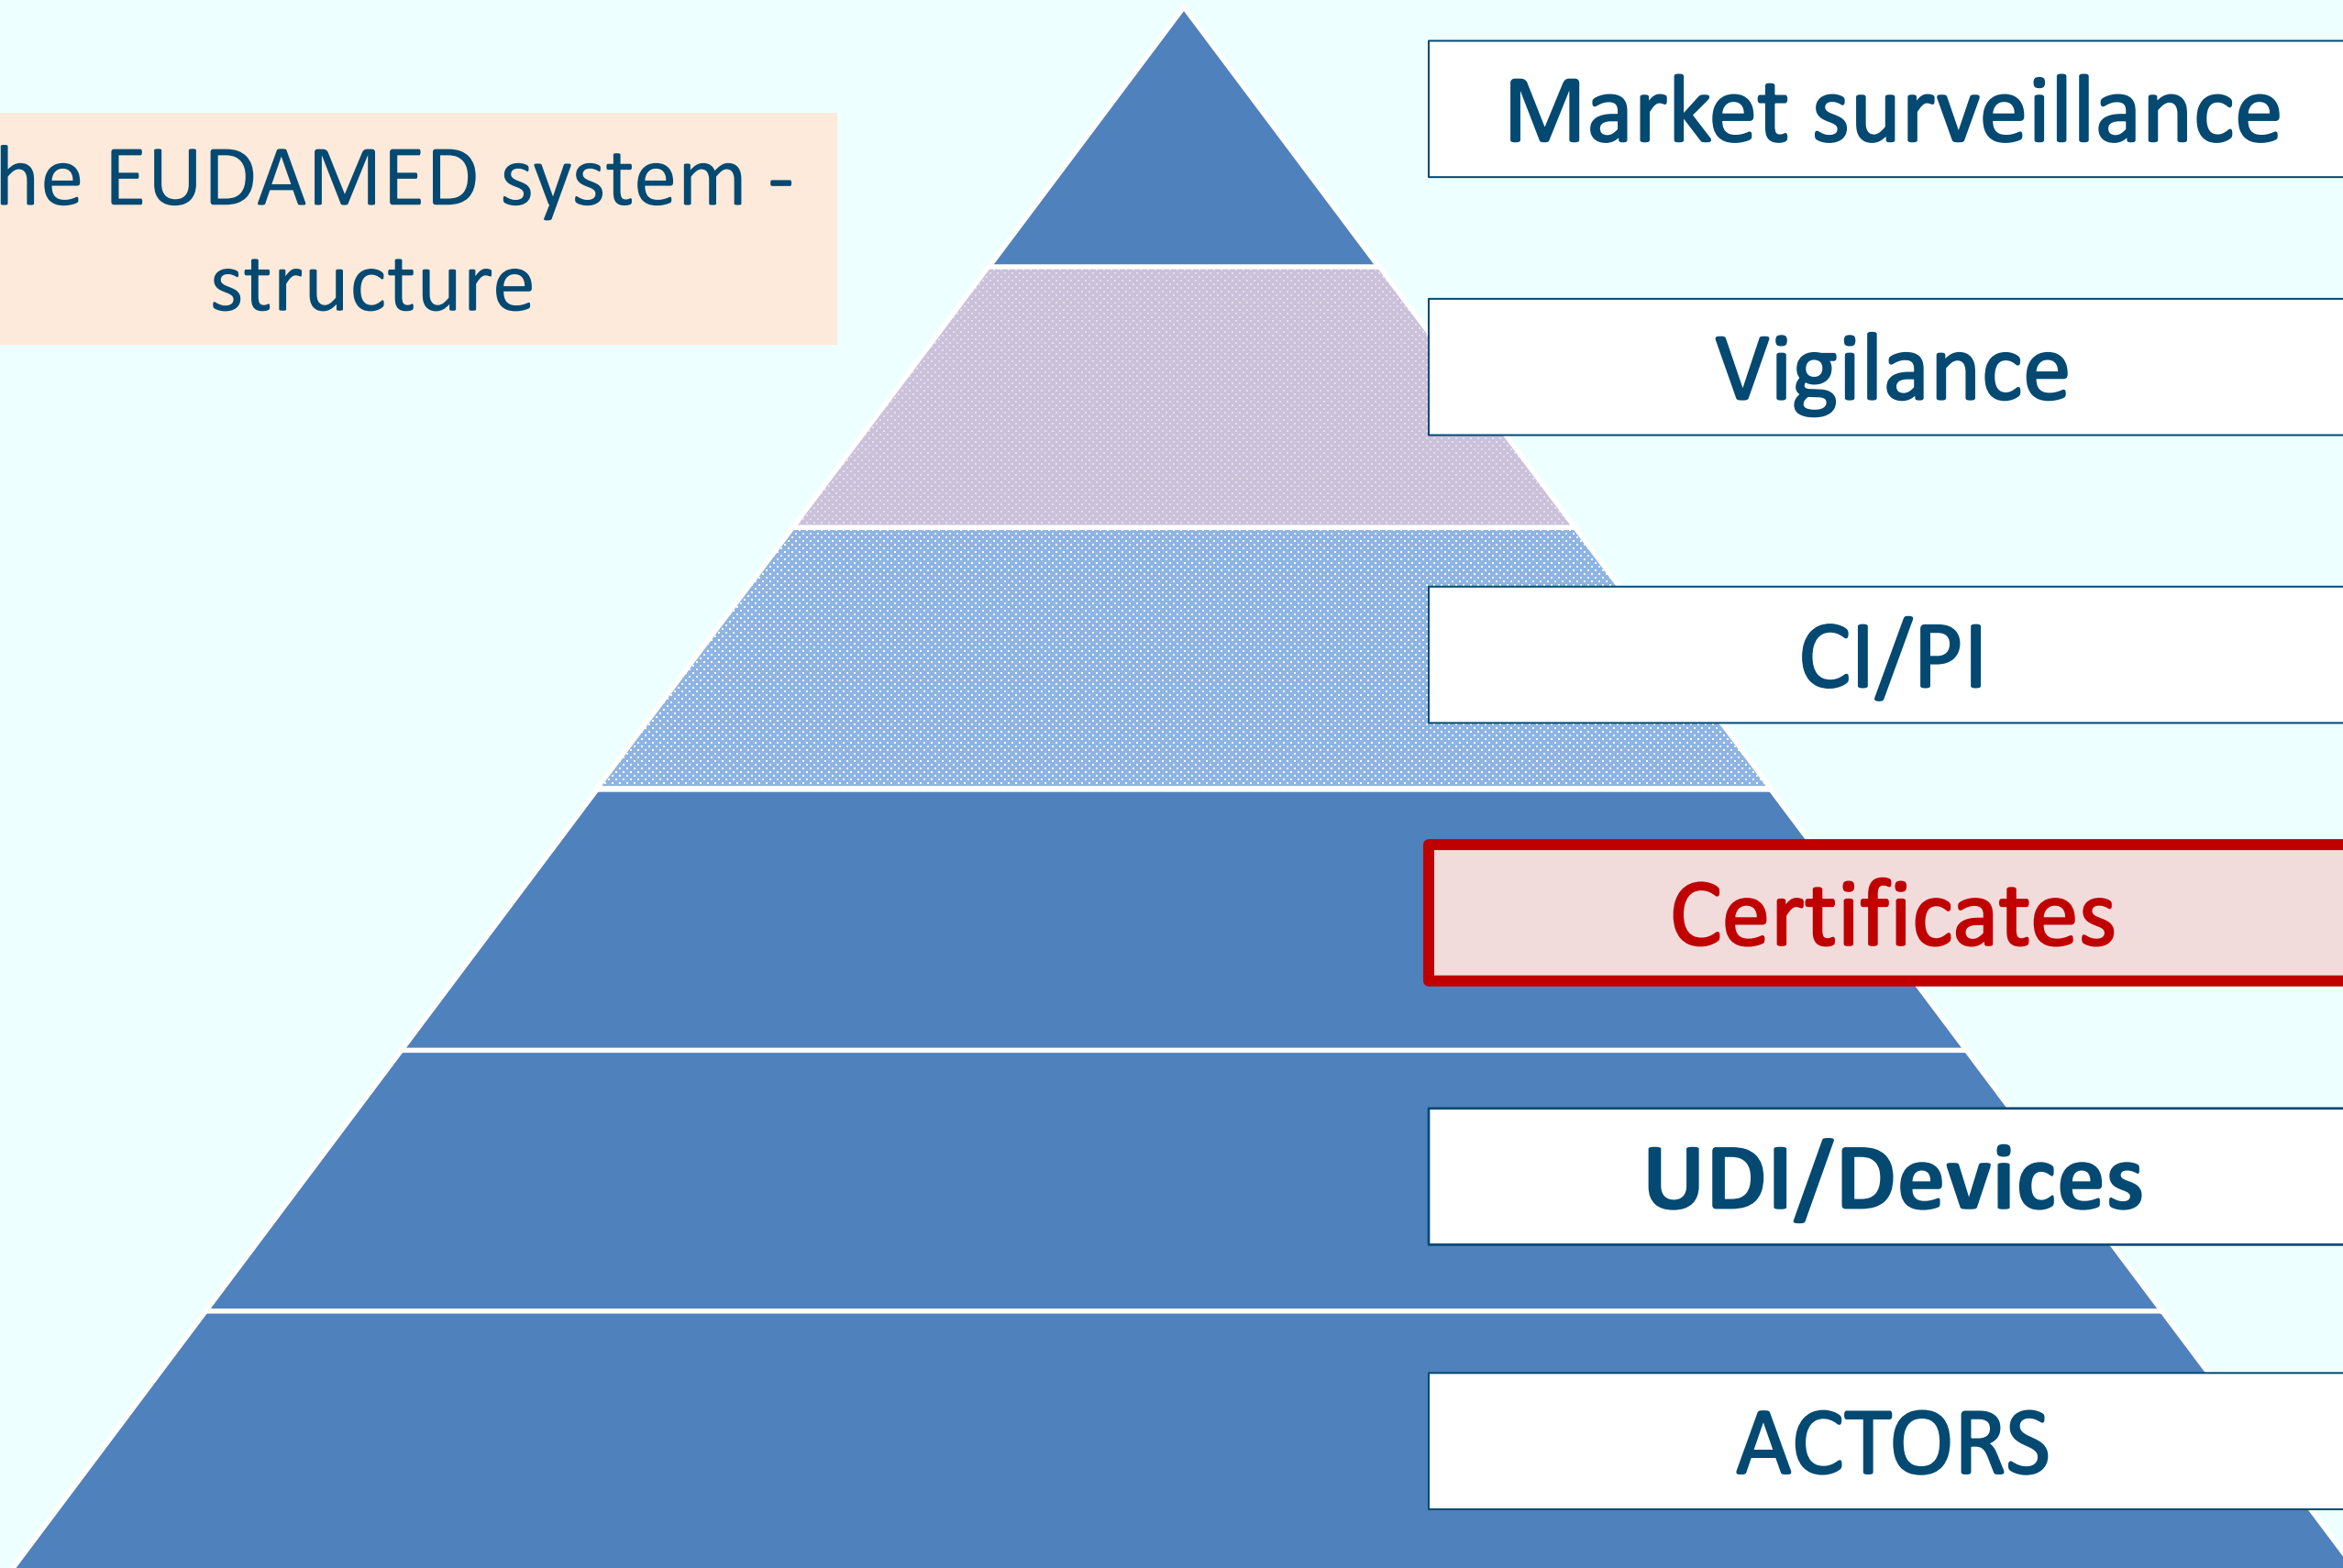

Vyhľadávanie certifikátu v EUDAMED

 Search for certificates and refused certificates

Search criteria

Search for:

Certificates Refused certificates

Certificate core data

Notified Body:

Certificate type:

Certificate number:

Certificate status:

Economic operator Actor ID/SRN:

Economic operator name:

Starting certificate validity date:

Special device properties:

Device data in the certificate

Device identification:

Enter the device identification value/text:

Risk class:



Podľa čísla certifikátu,
NB, SRN



Podľa pomôcky



Ďakujem za pozornosť !

Zuzana Baťová